

Supplymentary Data

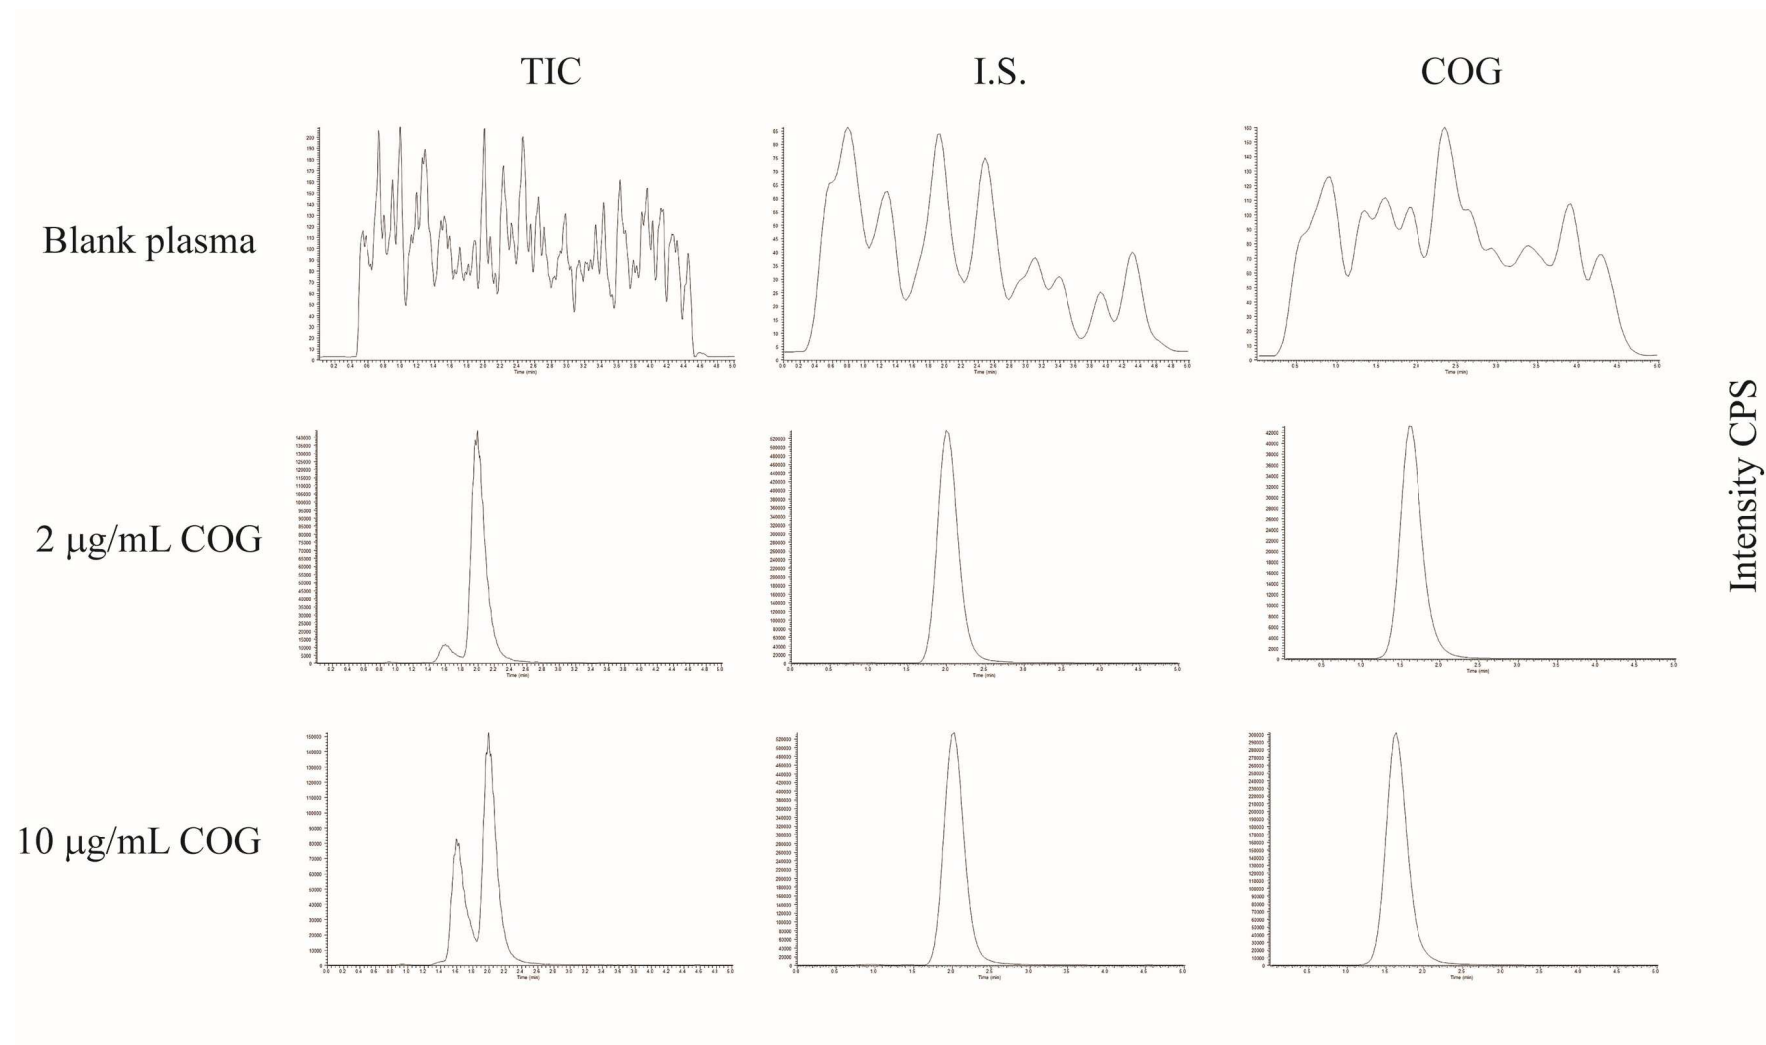


Fig. S1: The chromatograms of COG and the internal standard from COG stability-test mouse plasma samples. The total ion current (TIC) chromatogram and extracted ion chromatograms of mouse plasma spiked with 1000 ng/mL I.S. and 2 µg/mL or 10 µg/mL COG are presented.